
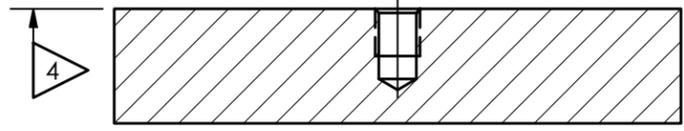
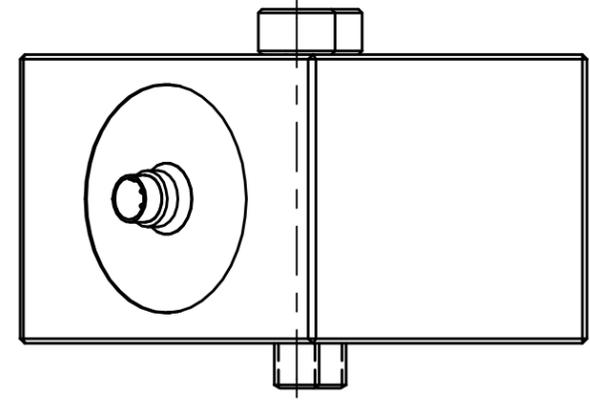
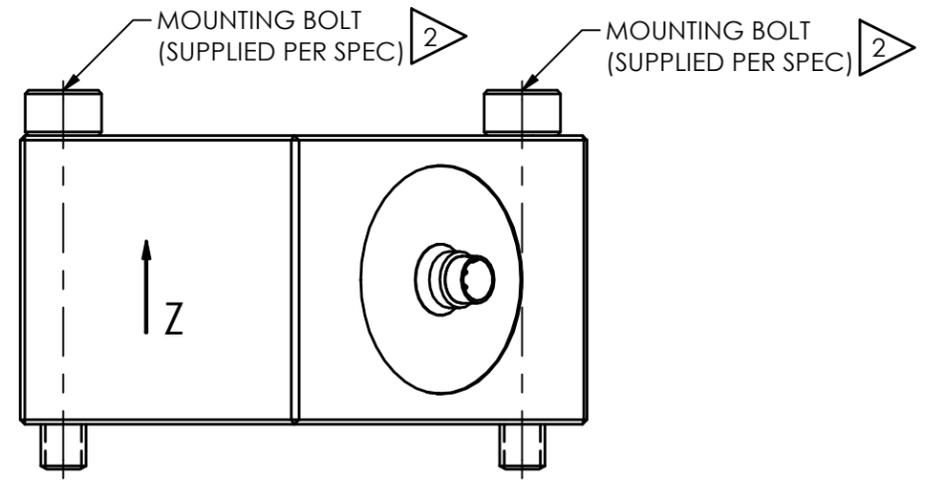


PCB Piezotronics Inc. claims proprietary rights in the information disclosed hereon. Neither it nor any reproduction thereof will be disclosed to others without the written consent of PCB Piezotronics Inc.

79990

REVISIONS		
REV	DESCRIPTION	DIN
NR	RELEASED TO DRAFTING	55536

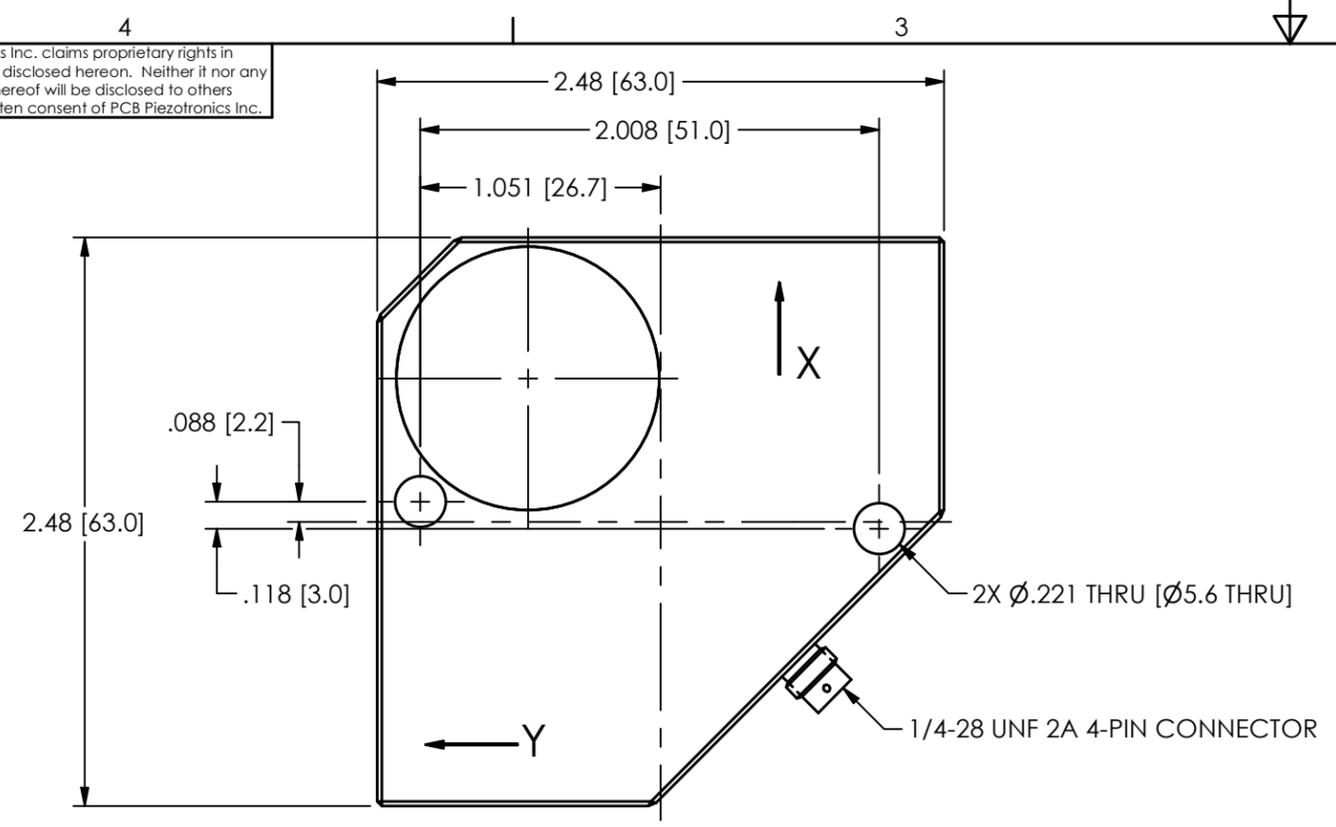

MOUNTING HOLE PREPARATION (2X):
M5x0.8-6g ∇ .205 [5.21] MIN

- 5.) FOR BEST RESULTS, PLACE A THIN LAYER OF SILICONE GREASE (OR EQUIVALENT) ON INTERFACE PRIOR TO MOUNTING
- 4 MOUNTING SURFACE SHOULD BE FLAT TO WITHIN .001 [.03] TIR ACROSS SENSOR FOOTPRINT WITH A FINISH OF 63 [1.61] OR BETTER FOR BEST RESULTS
- 3 DRILL PERPENDICULAR TO MOUNTING SURFACE TO WITHIN $\pm 1^\circ$
- 2 4 mm HEX: RECOMMENDED MOUNTING TORQUE OF 30 - 40 in-lb [3.4 - 4.5 Nm]
- 1.) MOUNTING BOLTS NOT SHOWN IN TOP VIEW FOR CLARITY

UNLESS OTHERWISE SPECIFIED TOLERANCES ARE:		DRAWN		CHECKED		ENGINEER		PCB PIEZOTRONICS			
DIMENSIONS IN INCHES		AME		JDM		DRK		AN AMPHENOL COMPANY			
DECIMALS XX \pm .01	DECIMALS X \pm 0.3	3/18/25	3/18/25	3/18/25	3/18/25	3425 WALDEN AVE. DEPEW, NY 14043			CODE IDENT. NO. 52681	SIZE B	DWG. NO. 79990
XXX \pm .005	XX \pm 0.13	TITLE		INSTALLATION DRAWING		3425 WALDEN AVE. DEPEW, NY 14043		SCALE: 1.25X			
ANGLES ± 2 DEGREES		CASE ISOLATED SEISMIC TRIAX				(716) 684-0001 E-MAIL: sales@pcb.com					
CABLE TOLERANCES IN ENGLISH											
CABLE TOLERANCES IN METRIC											
FILLETS AND RADII											
FILLETS AND RADII											